

FIG. 1

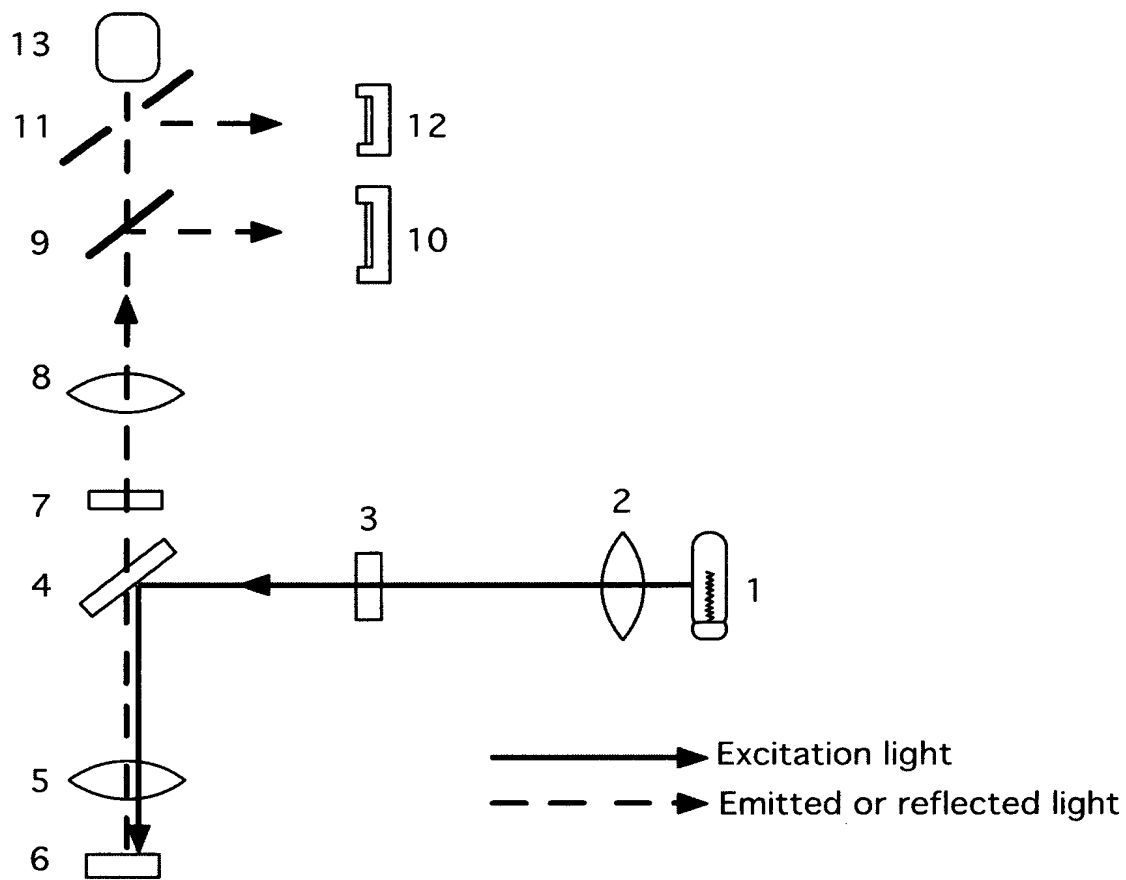


Figure 2. Schematic of microspectrometer and fluorescence detection system used to characterize the colorant dye loaded in microspheres.

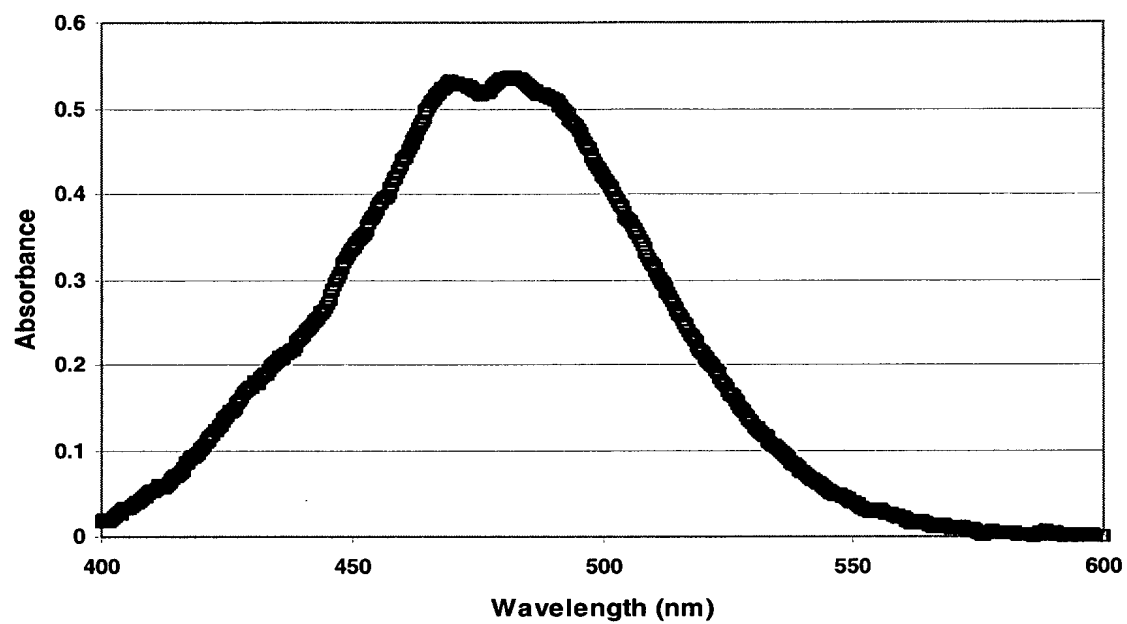


Figure 3. Spectroscopic response from a micro-sphere containing YD-1